

FIG. 2



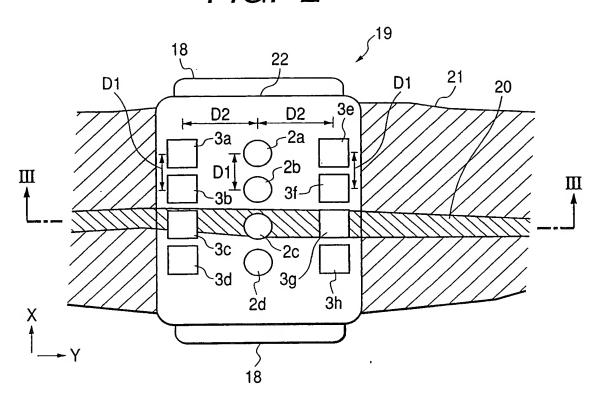


FIG. 3

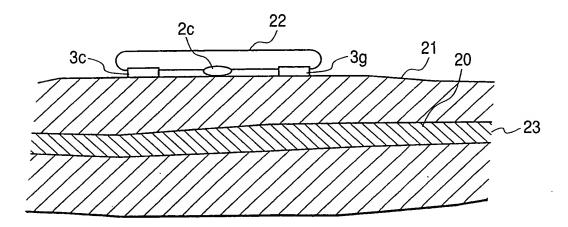

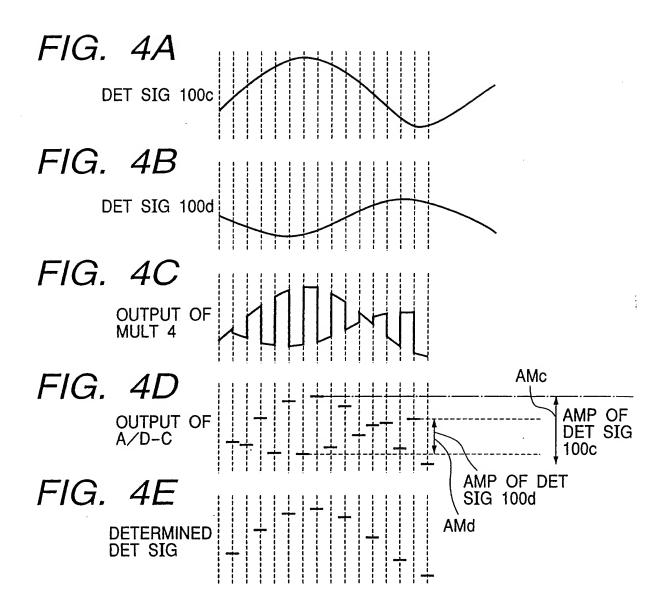

## FIG. 5A

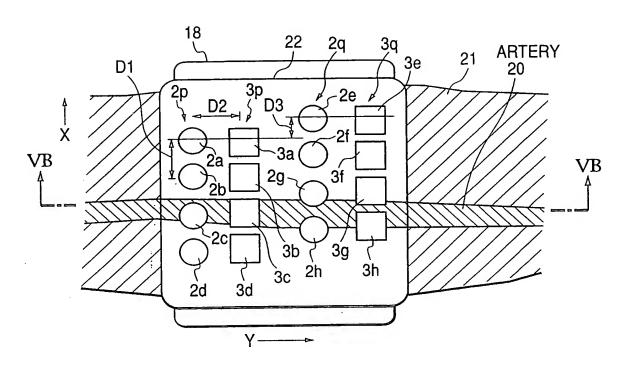
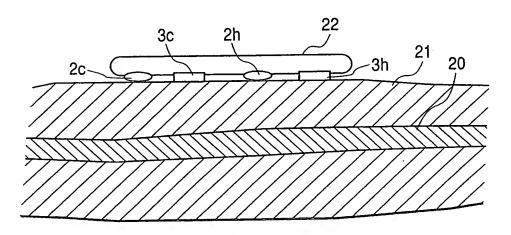
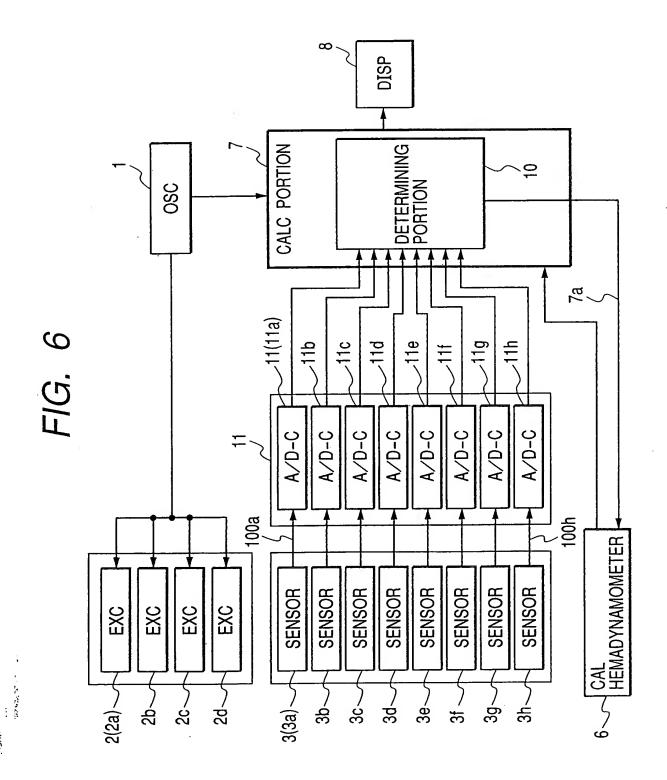
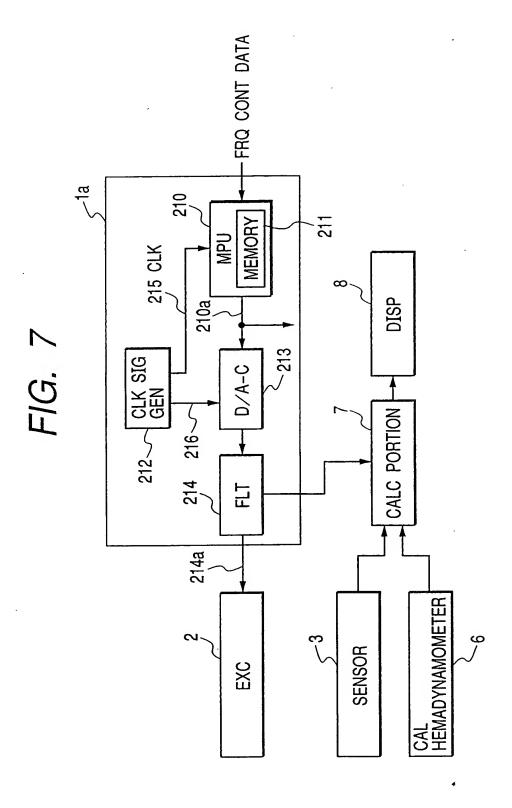


FIG. 5B







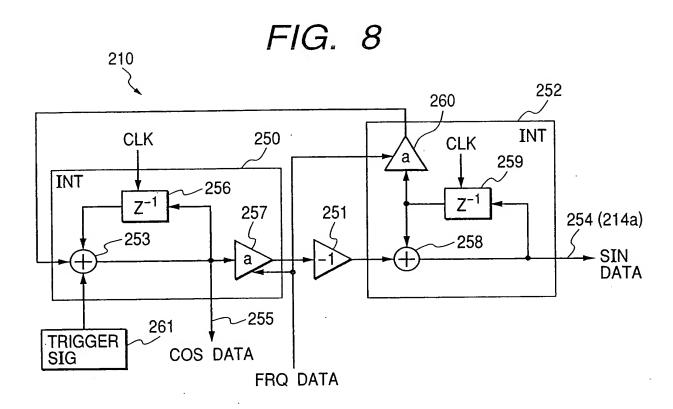


FIG. 9 \_1b 222 CLK SIG GEN 220 223 224 221-CLK NUMERICAL-CONTROLLED OSC FRQ CONT MPU **EXC** DATA -2 **SENSOR** CALC PORTION **DISP** CAL HEMADYNAMOMETER

FIG. 10 -232 ADDRESS GEN CLK SIG GEN 233-<del>5 235</del> -234 231 -230 **FRQ** LOOKUP-TABLE **MPU** CONT **EXC DATA SENSOR** CALC PORTION DISP CAL HEMADYNAMOMETER

FIG. 11

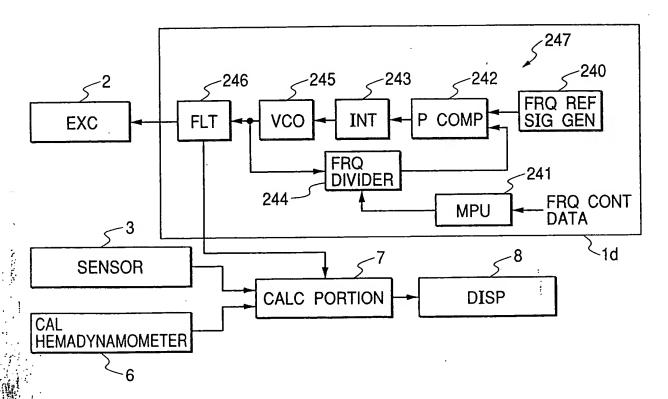


FIG. 12

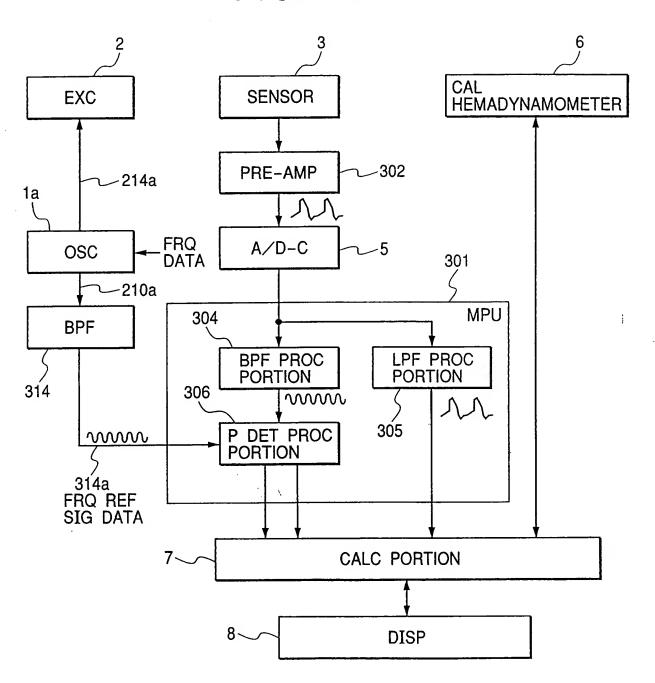


FIG. 13A

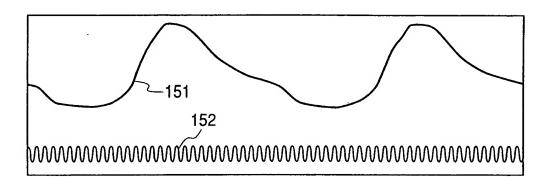


FIG. 13B

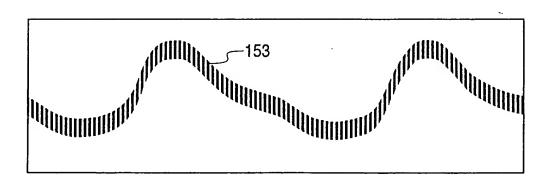
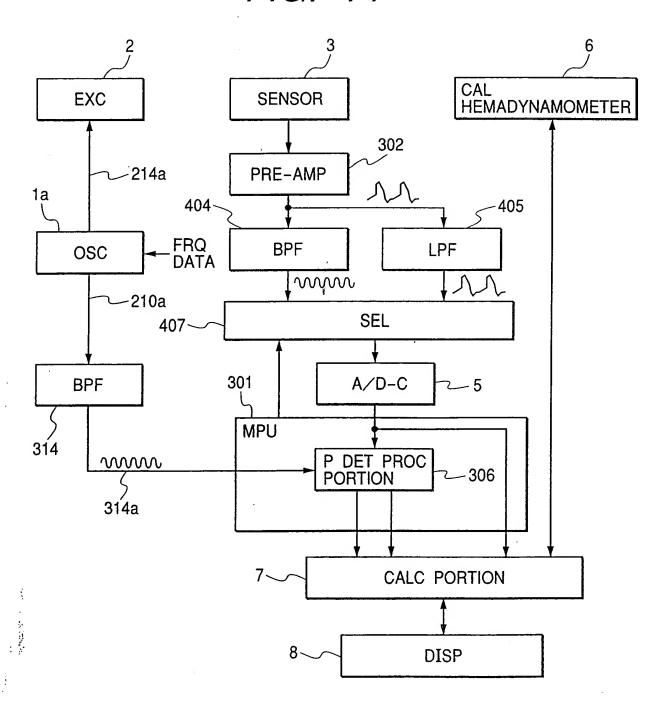


FIG. 14



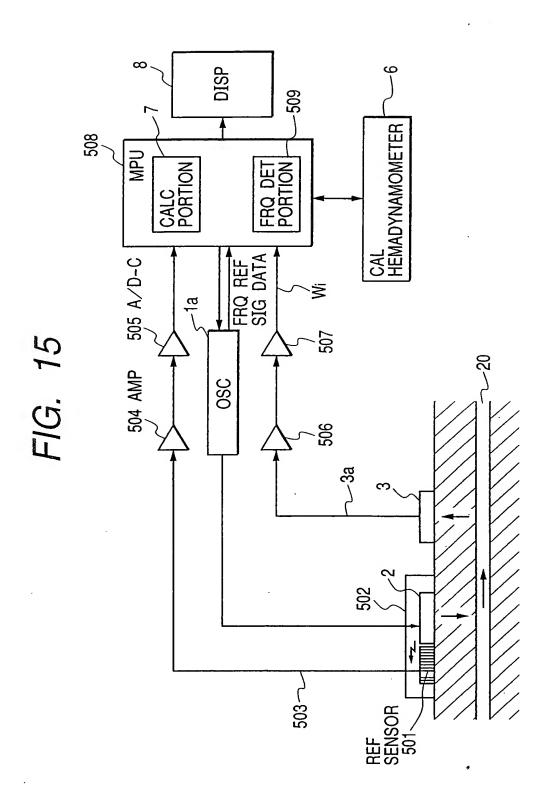




FIG. 16

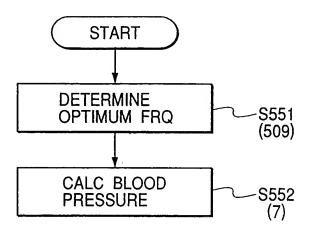


FIG. 18

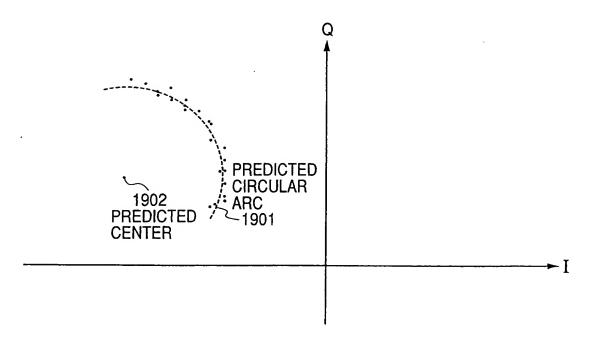
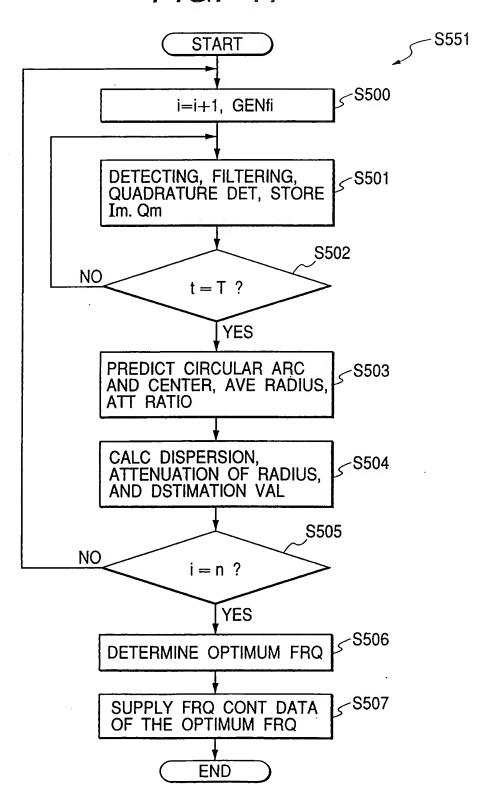


FIG. 17



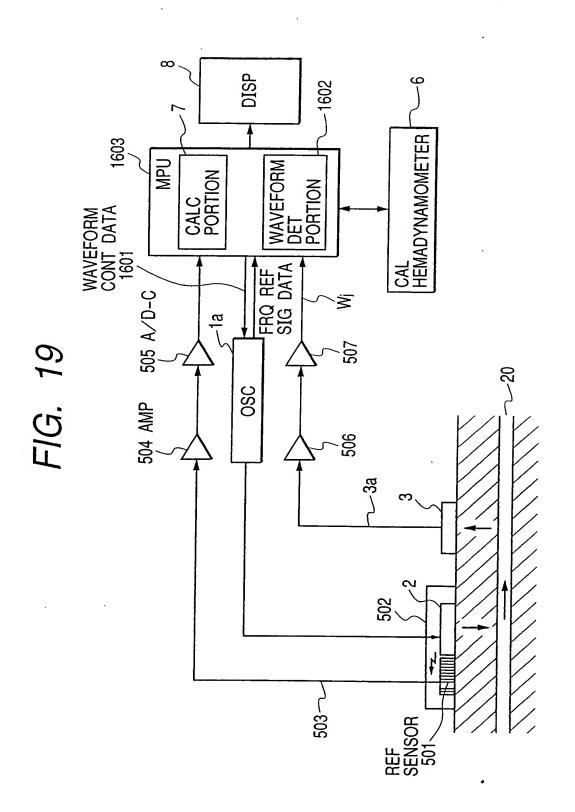


FIG. 20

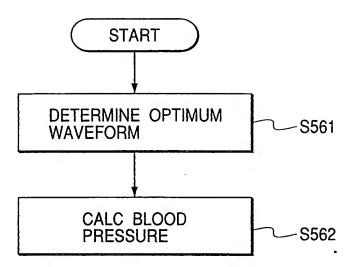


FIG. 21

